GS501DZ Tech Sheet

Balboa System PN 55250-01

System Model # GS5-GS501DZ-RCA-3.0 Software Version # 43 EPN # 2808

Base PCBA – PN 55251-01 PCB GS500Z – PN 22015 Rev B

Base Panels VL801D (Serial Deluxe) – PN 54121 VL802D – PN 54562





System Revision History

System PN	EPN	Date	Requested By	Changes Made	
55250-01	2808	01.26.2009	Balboa	Software update to version 43.	
55250-01	2808	02.05.2009	Balboa	Change Panels and add note to both circuit board setup.	

Page 2 55250-01_97_A

Basic System Features and Functions

Power Requirements

Single Service [3 wires (line, neutral, ground)]

• 230VAC, 50Hz, $1\sim$, 16A/32A, (Circuit Breaker rating = 20A/40A max.)

Dual Service [5 wires (line 1, neutral 1, line 2, neutral 2, ground)]

• 230VAC, 50Hz, 1~, 2x 16A, (Circuit Breaker rating = 20A max each service.)

3-Phase Service [5 wires (line 1, line 2, line 3, neutral, ground)] Requires PCB Rev B.

- 400VAC, 50Hz, 3N~, 16A, (Circuit Breaker rating = 20A max each phase line.)
- IMPORTANT Service must include a neutral wire, with a line to neutral voltage of 230VAC.

System Outputs

Setup 1 (As Manufactured)

- 230V Pump 1, 2-Speed
- 230V Blower
- 230V Ozone
- 10V Spa Light
- 230V AV (Stereo)
- 230V 3.0kW Heater *


Setup 2

- 230V Pump 1, 2-Speed
- 230V Blower
- 230V Ozone
- 230V Circ Pump
- 10V Spa Light
- 230V AV (Stereo)
- 230V 3.0kW Heater *

* Heater wattage is rated at 240V.

Additional OptionsFull Feature Dolphin Remote

- Full Feature Dolphin Remote and Spa-only Dolphin Remote
- IR Receiver Module Connects to terminal J1 or J2 (Must be 8-pin connector)
- MoodEFX Lighting Connects to Spa Light terminal J20
- FiberEFX Lighting
 Connects to Spa Light terminal J20

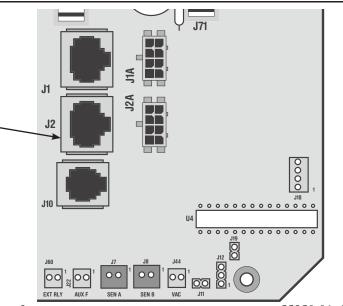

Page 3 55250-01_97_A

Basic System Features and Functions

Any time you change a DIP Switch, other than A1, you must reset Persistent Memory for your new DIP Switch Settings changes to take effect. If you do not reset Persistent Memory, your system may function improperly.


To reset Persistent Memory:

- Power down by disconnecting power source from spa.
- Put a jumper across J43, covering both pins. (See illustration below)
- Power up by connecting power source to spa.
- Wait until "Pr" is displayed on your panel.
- Power down again.
- Remove jumper from J43 (May also move to cover 1 pin only)
- Power up again.

About Persistent Memory and Time of Day Retention:

This system uses memory that doesn't require a battery to store a variety of settings. What we refer to as Persistent Memory stores the filter settings, the set temperature, and the heat mode.

Persistent Memory is not used for Time of Day. Only models with a Serial Deluxe panel installed (VS5xxDZ and GS5xxDZ) can display the time. However, during power loss to the spa, the system will lose the correct time, and reset to 12:00 PM when power is restored.

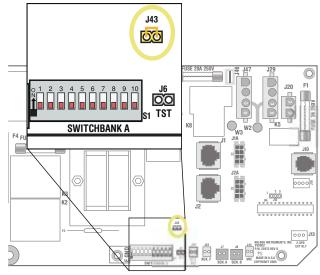

J43 on VS5xxZ and VS300 Series Main Board Shown. J43 on GS5xxZ Series is located in approximately the same position.

Power Up Display Sequence

Upon power up, you should see the following on the display:

- Displayed next is: "건너" (indicating the system is configured for a heater between 3 and 6 kW) or "¿¿"" (indicating the system is configured for a heater effectively* between 1 and 3 kW). "건너" should appear for all VS models running at 240VAC. "¿¿" should appear for all VS models running at 120VAC, as well as all GS models. (*A heater which is rated at 4 kW at 240VAC will function as a 1 kW heater at 120VAC.)
- "Pr" will appear to signal the start of Priming Mode.

At this point, the power up sequence is complete. Refer to the Reference Card for the VS or GS System model of your spa for information about how the spa operates from this point on, including how to adjust the Time of Day if using a Serial Deluxe style panel.

Wiring Configuration and DIP Settings


Setup 1 (As Manufactured)

- 230V Pump 1, 2-Speed
- 230V Blower
- 230V Ozone
- 10V Spa Light
- 230V AV (Stereo)
- 230V 3.0kW Heater

H_IPot Testing Note:

Disconnect slip terminal with green wires from J90 prior to performing HiPot test. Failure to disconnect may cause a false failure of the test.

Reconnect terminal to J90 after successful completion of HiPot test.

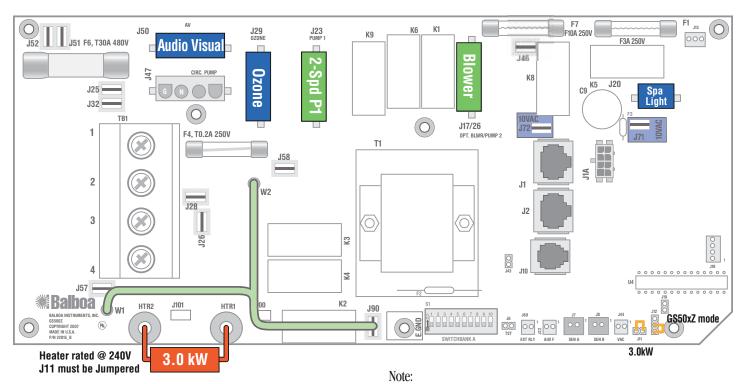

VL801D Main Panel

• When not using Blower, turn switch A7 off.

WARNING: Main Power to system should be turned OFF BEFORE adjusting DIP switches. WARNING: Persistent Memory (J43) must be RESET to allow new DIP switch settings to take effect. (See Persistent Memory page) Switchbank A GS500/501/510DZ Wiring Color Key SSID# Software 3 **Neutral (Common) AC Connections** J11 J12 ³ 100 3.0kW Special AC Connections 99 Heater **Line AC Connections** 43 10 Volt Connections A1, Test Mode OFF A6, 50 Hz **Relay Control Wires** A2, See Table 1 A7, J17/26 Enabled J43 A3, Exp Pump Disabled A8, Degrees C Memory **Board Connector Key** A4, Aux Freeze A9, Non-Circ Mode Reset A5, 2-speed P1 Typically Line voltage A10, See Table 1 Typically Line voltage for 2-speed pumps **Panel Button Positions** Panel Button Assignments Neutral (Common) 1=Time 5=Light 3 8 5 Ground 2=Mode/Prog 6=Pump 1 2 4 6 7 3=Temp Up 7=Unused Note flat sides in connector 4=Temp Down 8=J17/26

Wiring Configuration and DIP Settings


Setup 2

- 230V Pump 1, 2-Speed
- 230V Blower
- 230V Ozone
- 230V Circ Pump
- 10V Spa Light
- 230V AV (Stereo)
- 230V 3.0kW Heater
- VL801D Main Panel

HiPot Testing Note:

Disconnect slip terminal with green wires from J90 prior to performing HiPot test. Failure to disconnect may cause a false failure of the test.

Reconnect terminal to J90 after successful completion of HiPot test.

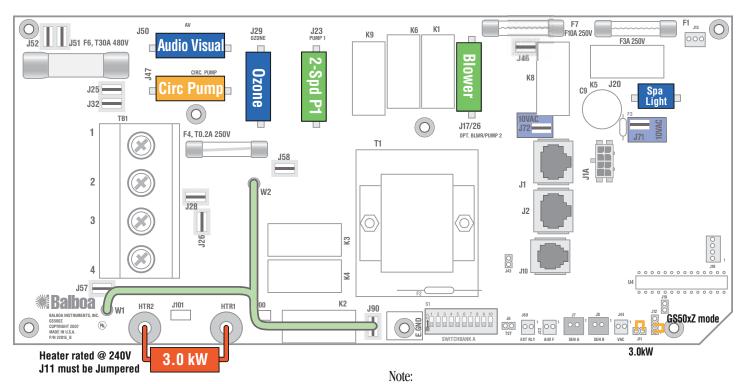

• When not using Blower, turn switch A7 off.

WARNING: Main Power to system should be turned OFF BEFORE adjusting DIP switches. WARNING: Persistent Memory (J43) must be RESET to allow new DIP switch settings to take effect. (See Persistent Memory page) Switchbank A GS500/501/510DZ Wiring Color Key SSID# Software 3 4 **Neutral (Common) AC Connections** J11 J12 ³ 100 3.0kW Special AC Connections 99 Heater **Line AC Connections** 43 10 Volt Connections A1, Test Mode OFF A6, 50 Hz **Relay Control Wires** A2, See Table 1 A7, J17/26 Enabled J43 A3, Exp Pump Disabled A8, Degrees C **Board Connector Key** Memory A4, Aux Freeze A9, 24 Hour 3°F Circ Pump Reset A5, 2-speed P1 Typically Line voltage A10, See Table 1 Typically Line voltage for 2-speed pumps **Panel Button Positions** Panel Button Assignments Neutral (Common) 1=Time 5=Light 3 8 5 Ground 2=Mode/Prog 6=Pump 1 4 6 7 3=Temp Up 7=Unused Note flat sides in connector 4=Temp Down 8=J17/26

DIP Switches and Jumpers Definitions

SSID 100 99 43 Base Model GS500DZ-GS501DZ-GS510DZ

DIP Switch Key

A1 Test Mode (normally OFF)

A2+A10 Control amp draw requirements (See Table 1) -

A3 "ON" position: Expander Board Enabled for 1-speed Pump only.

"OFF" position: Expander Board Disabled.

A4 Aux Freeze (must be OFF)

A5+A9 Pump 1 speeds and Circ Modes:

A5	A9	Circ Mode	Pump 1 Speed
OFF	OFF	Non-circ	2-speed
ON	OFF	Circ "acts like Pump 1 low" (filters/polls/ect)	1-speed
OFF	ON	24 hours with 3°F shut-off	1-speed
ON	ON	24 hours with 3°F shut-off	2-speed

of Hi-Speed Table 1 Pumps/Blower **Before Heat Disabled** <u>A2</u> A10 **OFF** 0FF 0 ON **OFF** 1 0FF ON 2 ON ON 3

A6 "ON" position: 50Hz operation "OFF" position: 60Hz operation

A7 "ON" position: J17/26 Enabled for Blower or 1-speed Pump.

"OFF" position: J17/26 Disabled

A8 "ON" position: temperature is displayed in degrees Celsius "OFF" position: temperature is displayed in degrees Fahrenheit

Jumper Key

J11 If using 3kW or higher wattage heater, jumper can be set in either position, but may perform better on Pins 1 and 2. If using 2.5kW or lower wattage heater, jumper must be set on 1 Pin only.

J12 Factory set. DO NOT MOVE.

Jumper must be on Pins 1 and 2 for GS51xZ/GS52xZ/GS5xxSZ/GS5xxDZ software. Jumper must be on Pins 2 and 3 for GS50xZ software.

Jumper must be on Pins 2 and 3 for G550x2 software.

When jumper is placed on 2 pins during power-up, system will reset persistent memory. Leave on 1 pin only to enable persistent memory feature.

WARNING:

- Setting DIP switches incorrectly may cause abnormal system behavior and/or damage to system components.
- Refer to Switchbank illustration on Wiring Configuration page for correct settings for this system.
- Contact Balboa if you require additional configuration pages added to this tech sheet.

Panel Button Positions



Panel Button Assignments

1=Time 5=Light 2=Mode/Proq 6=Pump 1

3=Temp Up 7=Expander Pump (when A3 is ON)

4=Temp Down 8=J17/26 (when A7 is ON)

Aux Panel Information

Supports 2-button aux panel


VX20 **6 7**

Supports 4-button aux panel

VX40D 6 7 8 5

Electrical Service Configuration Options

Systems with PCB Rev B Only

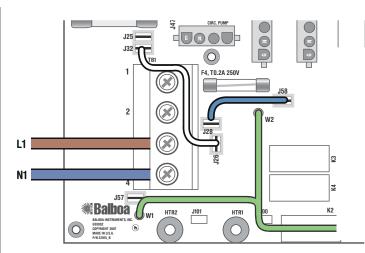

Single Service, TN and TT Electrical Systems (1 x 16 Amp or 1 x 32 Amp)

3 Wires (1 Line + 1 Neutral + 1 Protective Earth)

Protective Earth wire (Green/Yellow) must be connected to system ground terminal as marked.

This option is configured and shipped as the default.

All equipment (pumps, blower, and heater) runs on service line L1.

Systems using only 1 DIP switch (A10) for heat disable:


For 1 x 16 Amp Service:

DIP Switch A10 must be ON.

For 1 x 32 Amp Service:

Set DIP Switch A10 such that total system amperage draw never exceeds rated service input.

Systems using multiple DIP switches for heat disable: Refer to system Hot Sheet DIP Switch Definition page and set the switches shown in Table 1 such that total system amperage draw never exceeds rated service input.

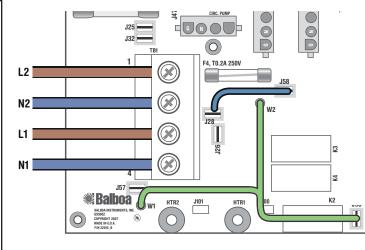

Dual Service, TN and TT Electrical Systems (2 x 16 Amp)

5 Wires (2 Lines + 2 Neutrals + 1 Protective Earth)

Protective Earth wire (Green/Yellow) must be connected to system ground terminal as marked.

The heater runs on service line L1, while all other equipment, such as pumps and blowers, run on service line L2.


Completely remove the white wire from J26 and J32. Note: J32 and J25 are electrically identical. The white wire may be attached to either terminal before removal.


Systems using only 1 DIP switch (A10) for heat disable: DIP Switch A10 must be OFF.

Systems using multiple DIP switches for heat disable: Refer to system Hot Sheet DIP Switch Definition page and set both switches shown in Table 1 to ON positions.

Electrical Service Configuration Options

Systems with PCB Rev B Only



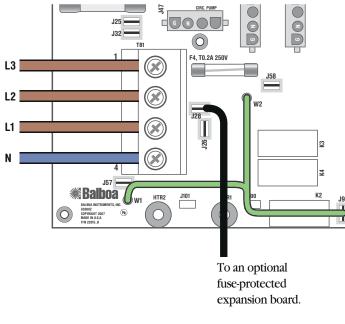

3-Phase Service, TN and TT Electrical Systems 5 Wires (3 Lines + 1 Neutral + 1 Protective Earth)

Protective Earth wire (Green/Yellow) must be connected to system ground terminal as marked.

IMPORTANT - Service MUST include a neutral wire, with a line to neutral voltage of 230VAC.

The heater runs on service line L1.

All main-board equipment run on service line L3. Additional equipment, such as expansion boards, run on service line L2.

Completely remove the white wire from J26 and J32, or J25. Completely remove the blue wire from J28 and J58.

If an expansion board is installed, black wire must connect to J28 (Line L2) only.

Systems using only 1 DIP switch (A10) for heat disable: DIP Switch A10 must be OFF.

Systems using multiple DIP switches for heat disable: Refer to system Hot Sheet DIP Switch Definition page and set both switches shown in Table 1 to ON positions.


NOTE:

- •Not all GS5xxZ systems can support 3-Phase.
- •3-Phase requires System PCB Rev B.
- If using an expansion board, the board must have fuse-protection.

Page 9 55250-01_97_A

Electrical Service Configuration Options

Systems with PCB Rev B Only

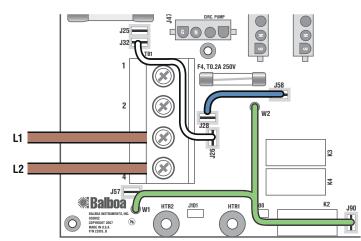

Single Service, IT Electrical System (No Neutral) Line - Line voltage is 230VAC (1 x 16 Amp or 1 x 32 Amp) 3 Wires (2 Lines + 1 Protective Earth)

Protective Earth wire (Green/Yellow) must be connected to system ground terminal as marked.

All equipment (pumps, blower, and heater) runs on service line L1 with L2 acting as the return.


Systems using only 1 DIP switch (A10) for heat disable: For 1 x 16 Amp Service:

DIP Switch A10 must be ON.

For 1 x 32 Amp Service:

Set DIP Switch A10 such that total system amperage draw never exceeds rated service input.

Systems using multiple DIP switches for heat disable: Refer to system Hot Sheet DIP Switch Definition page and set the switches shown in Table 1 such that total system amperage draw never exceeds rated service input.

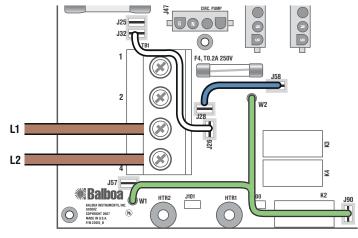

Line 3 - Cap (Insulate) end, Do not connect.

3-Phase Service, IT Electrical System (No Neutral) Line - Line voltage is 230VAC 4 Wires (3 Lines + 1 Protective Earth)

Protective Earth wire (Green/Yellow) must be connected to system ground terminal as marked.

All equipment (pumps, blower, and heater) runs on service line L1 with L2 acting as the return.

Systems using only 1 DIP switch (A10) for heat disable: For 1×16 Amp Service:

DIP Switch A10 must be ON.

For 1 x 32 Amp Service:

Set DIP Switch A10 such that total system amperage draw never exceeds rated service input.

Systems using multiple DIP switches for heat disable: Refer to system Hot Sheet DIP Switch Definition page and set the switches shown in Table 1 such that total system amperage draw never exceeds rated service input.

NOTE:

L3


- Not all GS5xxZ systems can support 3-Phase.
- •3-Phase requires System PCB Rev B.
- If using an expansion board, the board must have fuse-protection.


Page 10 55250-01_97_A

Ozone Connections

Note: A special tool is required to remove the pins from the connector body once they are snapped in place. Check with your Balboa Account Manager for information on purchasing a pin-removal tool.


Balboa Ozone connector configuration for 230VAC 50Hz:



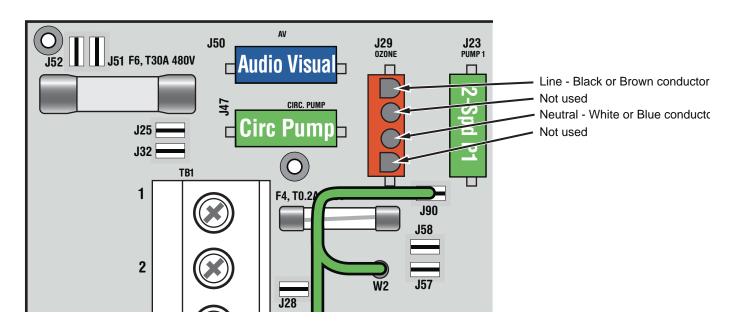


Page 11 55250-01_97_A

Serial Deluxe Panel Configurations

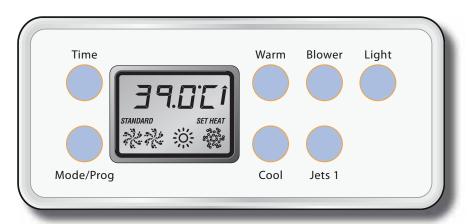

VL801D (Serial Deluxe) PN 54121 with no Overlay

• Connects to Main Board terminal J1 only*

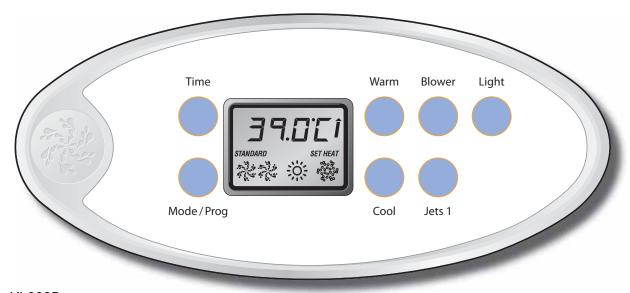

VL802D

PN 54562 with no Overlay

• Connects to Main Board terminal J1 only*

^{*} Panels with back-lighting (bulbs installed) should never be plugged into J2. Use J1 only. If the backlight bulbs are removed, then both J1 and J2 may be used.